



ieMR Advanced

Continuous infusions: NIKI pump (subcutaneous infusion) – discontinue and commence new infusion from new order


Medication Management

Quick reference guide



Discontinue and New Infusion

1. Click **MAR** from the **Menu**.
2. Locate the discontinued infusion in the **Discontinued Continuous Infusions** section.


Note: Ensure the **MAR filter** is set to **All Medications (System)**.

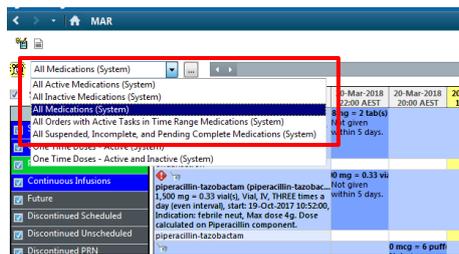


3. Right **Click** on the order and select **'Additional Dose'**.

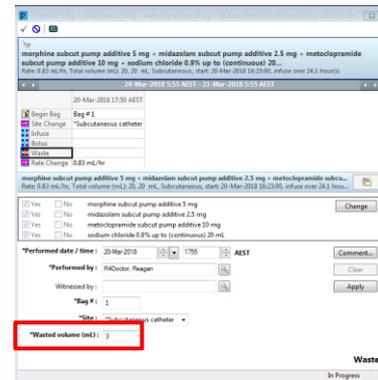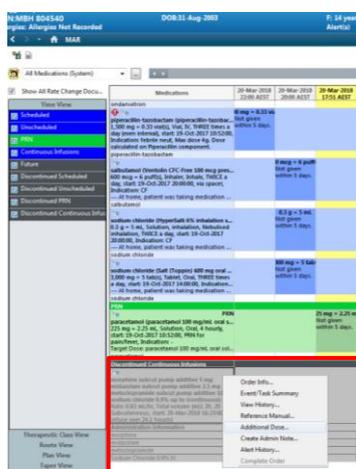

3. Select **Waste** and enter the volume being discarded as identified on the syringe driver in the **'Wasted volume (mL)'** field.
4. Type the witness' last name in the **'Witnessed by'** field.
5. Click **Apply** and enter the witness' password in the verify user window and select the green tick ✓.
6. **Refresh** the **MAR**.
7. Locate the new Continuous Infusion order.

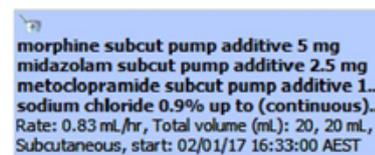

8. Expand the order sentence box by dragging it out.

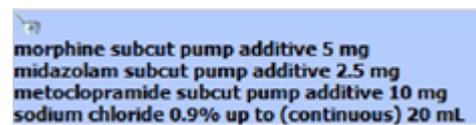


This will allow the dose of each medication to be viewed.

9. Select the **Tear Off** function in the toolbar.

The **Tear Off** function allows you to view two pages within **PowerChart** on the same screen, this is essential when documenting a NIKI.



10. With the now smaller **MAR** window, scroll down through the **MAR** to locate the NIKI order, then drag the **MAR** window to the right side of the screen.
11. Select **Interactive View** from the **Menu**.
12. Navigate to the **Paediatric Lines- Devices** band.
13. Right click on the previous NIKI pump dynamic group and select Inactivate.
10. Create a new **dynamic group** for the new infusion by selecting the dynamic group icon  next to **Subcutaneous Infusion Device**.
11. Select NIKI, enter the site and laterality and select **OK**.
12. Complete all relevant information required for documenting the administration of a NIKI under the newly created dynamic group heading using the **MAR** tear off page (example below).

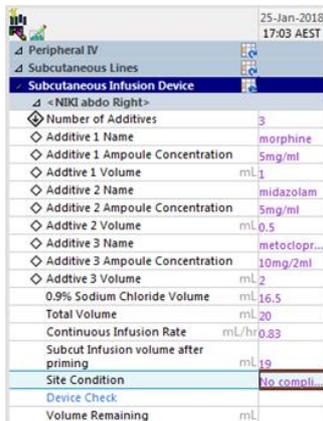



Note, the continuous infusion rate that you are documenting in iView is the rate displayed on the NIKI pump. It should be comparable to the ordered rate.

14. Select the  to sign off the documentation in **Interactive View**.

15. Type the witness' last name in the **Witnessed By** field.



16. Use the  to locate the witness' name in the system, and then select **OK**.
17. The witness will now check the entered information then click **Witness Sign** to co-sign the NIKI documentation.
18. Reattach the tear-off using the  **Attach** button.
19. Perform allergy check and **mark as reviewed**.
20. Navigate to the **MAW** and perform PPID check and barcode scanning.
21. Select the checkbox beside the order and then click in the results column to open the administration window.

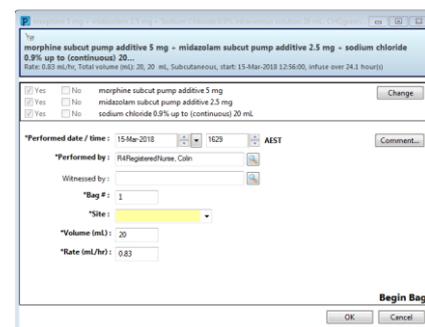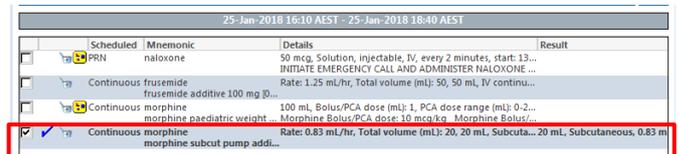

22. Enter the **site** and nurse witness and select **OK**.
23. **Nurse witness** to enter password.
24. Select sign and refresh the **MAR**.

