

Output – modify documented output

SAAnaesthesia

Quick reference guide

A recorded **Output** can be modified in multiple ways within **SAAnaesthesia**:


- Right click function – right clicking the documented **Output** dot (not the numerical value), presents the user with a drop down menu to select either **Modify** or **Remove**, selecting the **Modify** option launches the **Modify Output** window.
- Left click function – left clicking on the documented **Output** dot (not the numerical value) launches the **Modify Output** window for the **Output** selected. Alternatively the **Output** component button on the **Toolbar** can be used to make any required modifications.

Modify a Documented Output via the Anaesthetic Record Grid

1. Either left click the documented **Output** dot or right click the **Output** dot and select the **Modify Output** option.

Output	Nasogastric fluid - AN	50 mL	
	Estimated Blood Loss - AN	100 mL	
	Urine Output - AN	120 mL	120

The **Modify Output** window launches.

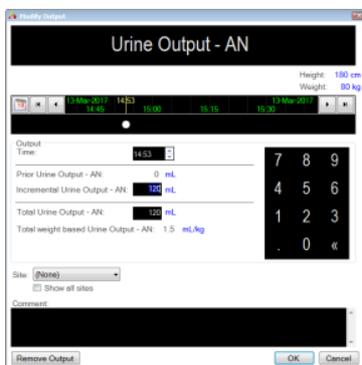

2. Within the **Modify Output** window edit the required data such as the **Output Volume**, the **Time**, or the **Site**. Note, the option of clicking to select the **Remove Output** button.
3. Click **OK** to complete the modifications and display the changes on the **Anaesthetic Record Grid**.

The **Modified Output** now populates the **Anaesthetic Record Grid**:

Urine Output - AN	165 mL	165
-------------------	--------	-----


Modify a Documented Output via the Output Button on the Toolbar

The **Output** component button on the **Toolbar** can be utilised to document the **Output** modifications:


1. Click the **Output** button on the **Toolbar**.



The **Select Output** window displays:

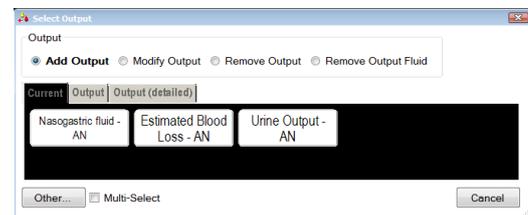


2. Click to select the **Modify Output** radio button.

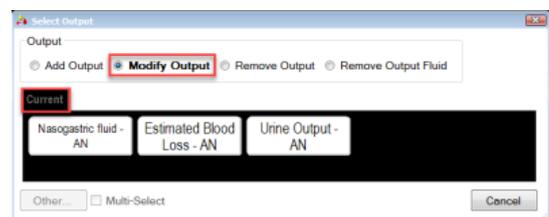

Note, the **Output** tabs are removed and the **Current** tab remains where all currently documented **Outputs** are displayed.

3. Click to select the **Output** button that requires modification.

The **Modify Output** window launches:

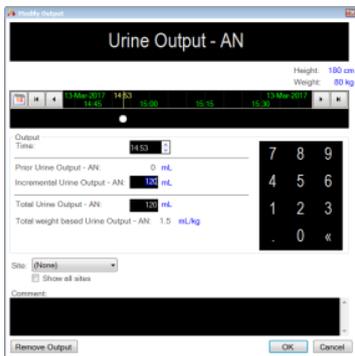

4. Within the **Modify Output** window edit the required data such as the **Output Volume**, the **Time**, or the **Site**. Note, the option of clicking to select the **Remove Output** button.
5. Click **OK** to complete the modifications and display the changes on the **Anaesthetic Record Grid**.

The **Modified Output** now populates the **Anaesthetic Record Grid**:



Note: Output volumes documented in SAAnaesthesia will flow into PowerChart - Interactive View Fluid Balance Navigator band in five minute intervals provided the data has not been modified for the past thirty minutes, or all volumes will populate the Fluid Balance Navigator band on finalisation of the SAAnaesthesia document.

